Tips and Tricks of HPLC System Troubleshooting

Agilent Technologies, Inc.

LC Tips And Tricks Seminar Series

Agilent Technologies

Trouble Shooting Steps

You Have Recognized There is a Problem!

How Do You Fix It?

- 1st Did System Suitability or Sample Fail?
- 2nd Review Method for Compliance
  - Is The Procedure Being Followed Properly?
  - Are Instrument Settings Correct?
- 3rd Ask More Questions!
  - When Did the System Last Function Properly?
  - Has Anything Been Changed?
- 4th Review ALL parameters!
  - The Obvious Is Not Always the Cause
  - Was There More Than One Change?

Agilent Technologies

HPLC System Components

Pump
Injector/Autosampler
Column
Detector
Data System/Integrator

Problems Can Be Related to All Components in the System

Agilent Technologies

Categories of Column and System Problems

A. Pressure

B. Peak shape

C. Retention

Agilent Technologies

Pressure Issues

Column Observations	Potential Problems
High pressure	- Plugged frit
	- Column contamination
	- Plugged packing
Low Pressure	- Leak
	- Flow Incorrect

Determining the Cause and Correcting High Back Pressure

- Check pressure with/without column - many pressure problems are due to blockages in the system or guard col.
  - Remove Column - Pressure Still High?
  - Remove Guard – Pressure Still High?
- ***If Column pressure is high:***
- Back flush column – Clear "dirty" frit surface
- Wash column – Eliminate column contamination and plugged packing
  - high molecular weight/adsorbed compounds
  - precipitate from sample or buffer

Change frit – Clear plugged frit ***PREVENT THIS!***

Column Cleaning

Flush with stronger solvents than your mobile phase.

Reversed-Phase Solvent Choices
in Order of Increasing Strength

Use at least 25 mL of each solvent for analytical columns

This Is Time Consuming

Often Performed Offline

- Mobile phase without buffer salts
- 100% Methanol
- 100% Acetonitrile
- 75% Acetonitrile:25% Isopropanol
- 100% Isopropanol
- 100% Methylene Chloride*
- 100% Hexane*

Must Reverse to Re-Equilibrate

*Tip: When using either Hexane or Methylene Chloride the column must be flushed with Isopropanol before returning to your reversed-phase mobile phase.

Agilent Technologies

Changing a Frit May Not Be a Good Idea

May not be possible with new generation columns
May damage high performance columns

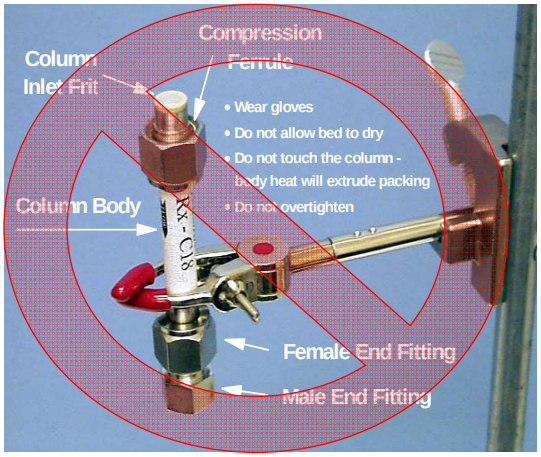
Compression Ferrule
Column Inlet Frit
• Wear gloves
• Do not allow bed to dry
• Do not touch the column - body heat will extrude packing
• Do not overtighten
Column Body
Female End Fitting
Male End Fitting

Tip: Prevention is a Much Better Idea!

Agilent Technologies

The Trick:
Prevention Techniques - A Better Choice!

- Use column protection
  - In-line filters
  - Guard columns
- Filter samples
- Filter buffered mobile phases

Easy

- Sample clean-up (i.e. SPE)
- Appropriate column flushing

Not As Easy

Inexpensive Filters Prevent Column Frit Plugging

Regenerated Cellulose (RC) Recommended

•Universal hydrophilic membrane, compatible with most solvents - aqueous and organic
•High purity, extremely low extractables and binding
•More Uniform Surface
•*Different than Other Cellulose Filters!!*



In-line Filters Easy to Use and replace

Frits Available in 0.2,0.5 and 2.0µ Porosity

Much Less expensive than a Column

Easier and Faster to Replace than a Column Frit



What Are Common Peak Shape Issues?

1. Split peaks
2. Peak tailing
3. Broad peaks

• Many peak shape issues are also combinations - i.e. broad and tailing or tailing with increased retention

•Symptoms do not necessarily affect all peaks in the chromatogram

•Each of these problems can have multiple causes

Agilent Technologies

Peak Splitting Caused By Disrupted Sample Path

•Flow Path Disrupted by Void

•Sample Allowed to Follow Different Paths Through Column

•Poorly Packed Bed Settles in Use

•High pH Dissolves Silica

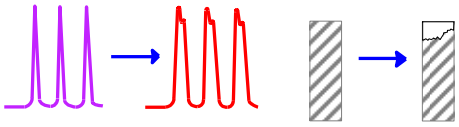

Normal **Double Peaks**

Split or Double Peaks

Tip: Similar Effect Can be Caused by Partially Plugged Frit

Agilent Technologies

Split Peaks from Column Contamination

Column: StableBond SB-C8, 4.6 x 150 mm, 5 µm Mobile Phase: 60% 25 mM Na_2HPO_4, pH 3.0 : 40% MeOH Flow Rate: 1.0 mL/min
Temperature: 35°C Detection: UV 254 nm Sample: Filtered OTC Cold Medication: 1. Pseudoephedrine 2. APAP 3. Unknown 4. Chlorpheniramine

Injection 1



Injection 30



Injection 1 After Column Wash with 100% ACN



Tip: Column washing eliminates the peak splitting, which resulted from a contaminant on the column
How could this be prevented? (Guard Column, SPE clean up of samples, Periodic column wash)

Agilent Technologies

Split Peaks from Injection Solvent Effects

Column: StableBond SB-C8, 4.6 x 150 mm, 5 µm Mobile Phase: 82% H_2O : 18% ACN
Injection Volume: 30 µL Sample: 1. Caffeine 2. Salicylamide

A. Injection Solvent 100% Acetonitrile



B. Injection Solvent Mobile Phase

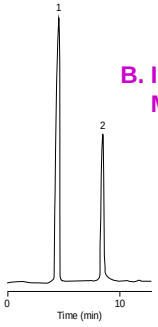

Tip: Injecting in a solvent stronger than the mobile phase can cause peak shape problems such as peak splitting or broadening
Trick: Keep Organic Concentration in Sample Solvent ≤ Mobile Phase

Agilent Technologies
Group/Presentation Title
Agilent Restricted
September 10, 2008Month
20XX

Peak Tailing, Broadening and Loss of Efficiency

May be caused by:

- Column "secondary interactions"
- Column contamination
- Column aging
- Column loading
- Extra-column effects

Agilent Technologies

Peak Shape: Tailing Peaks

Symmetry > 1.2



Normal Tailing



Normal Tailing

Causes

Some Peaks Tail:

- Secondary - Retention Effects.
- Residual Silanol Interactions.
- Small Peak Eluting on Tail of Larger Peak.

All Peaks Tail:

- Extra-Column Effects.
- Build up of Contamination on Column Inlet.
- Heavy Metals.
- Bad Column.

Agilent Technologies

Peak Tailing

Identifying Column "Secondary Interactions"

Column: Alkyl-C8, 4.6 x 150 mm, 5µm Mobile Phase: 85% 25 mM Na_2HPO_4 pH 7.0 : 15% ACN Flow Rate: 1.0 mL/min
Temperature: 35°C Sample: 1. Phenylpropanolamine 2. Ephedrine 3. Amphetamine 4. Methamphetamine 5. Phenteramine

No TEA

USP TF (5%)

1. 1.29
2. 1.91
3. 1.63
4. 2.35
5. 1.57

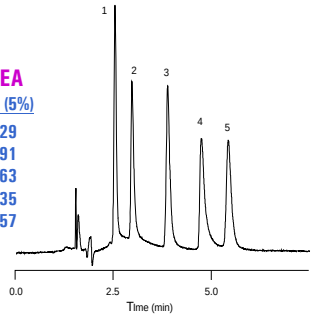

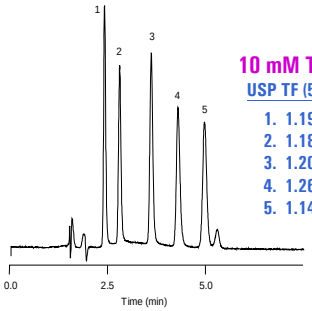

10 mM TEA

USP TF (5%)

1. 1.19
2. 1.18
3. 1.20
4. 1.26
5. 1.14

Tip: Mobile phase modifier (TEA) competes with Sample for surface ion exchange sites at mid-range pH values

Agilent Technologies

Peak Tailing

Low pH Minimizes "Secondary Interactions" for Amines

Column: Alkyl-C8, 4.6 x 150 mm, 5µm Mobile Phase: 85% 25 mM Na_2HPO_4 : 15% ACN Flow Rate: 1.0 mL/min
Temperature: 35°C Sample: 1. Phenylpropanolamine 2. Ephedrine 3. Amphetamine 4. Methamphetamine 5. Phenteramine

pH 3.0

USP TF (5%)

4. 1.33

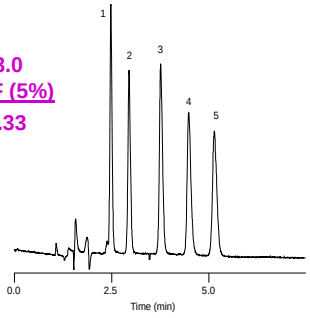

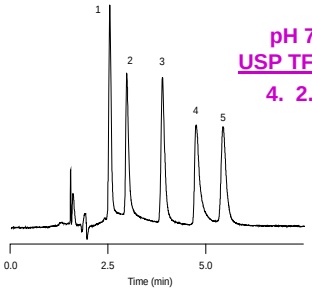

pH 7.0

USP TF (5%)

4. 2.35

Tip: Reducing mobile phase pH reduces interactions with silanols and peak tailing.

Agilent Technologies

Peak Tailing

High pH Eliminates "Secondary Interactions" for Amines

Column: ZORBAX Extend-C18, 4.6 x 150 mm, 5 m m Mobile Phase: See Below Flow Rate: 1.0 mL/min Temperature: RT
Detection: UV 254 nm
Sample 1. Maleate 2. Scopolamine 3. Pseudoephedrine 4. Doxylamine 5. Chlorpheniramine 6. Triprolidine 7. Diphenhydramine

pH 7
30% 20 mM Na_2HPO_4
70% MeOH



t_R = 8.5

pH 11
30% 20 mM TEA
70% MeOH

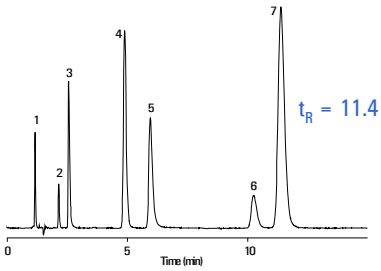

t_R = 11.4

Peak Shape and Retention of this sample of basic compounds improves at high pH where column has high IEX activity. *Why?*

Agilent Technologies

Peak Tailing - Column Contamination

Tip: Quick Test to Determine if Column is Dirty or Damaged

Trick: Reverse Column and Run Sample –If Improved, Possible Cleaning Will Help -No improvement-Column Damaged and Needs to be Replaced

QC test forward direction

	Plates	TF
1.	7629	2.08
2.	12043	1.64
3.	13727	1.69
4	13355	1.32

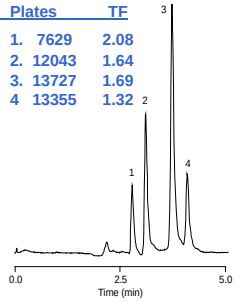

QC test reverse direction

	Plates	TF
1.	7906	1.43
2.	12443	1.21
3.	17999	1.19
4	17098	1.25



QC test after cleaning 100% IPA, 35°C

	Plates	TF
1.	7448	1.06
2.	12237	1.21
3.	15366	1.11
4	19067	1.17

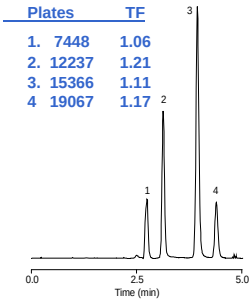

Column: StableBond SB-C8, 4.6 x 250 mm, 5µm Mobile Phase: 20% H_2O : 80% MeOH Flow Rate: 1.0 mL/min
Temperature: R.T. Detection: UV 254 nm Sample: 1. Uracil 2. Phenol 3. 4-Chloronitrobenzene 4. Toluene

Agilent Technologies

Peak Shape: Fronting Peaks

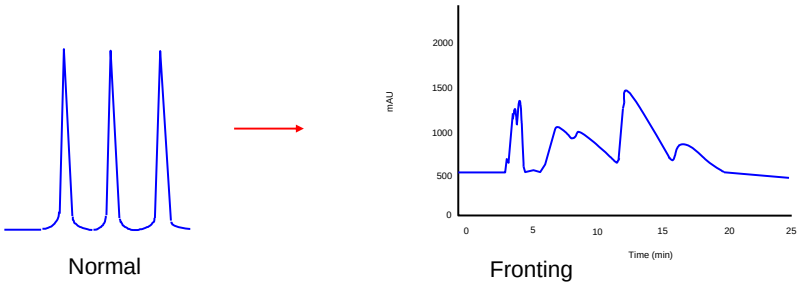

Normal

Fronting

Symmetry < 0.9

Causes:

- Column Overload

Agilent Technologies

Peak Tailing/Broadening
Sample Load Effects

Columns: 4.6 x 150 mm, 5µm Mobile Phase: 40% 25 mM Na_2HPO_4 pH 7.0 : 60% ACN Flow Rate: 1.5 mL/min
Temperature: 40°C Sample: 1. Desipramine 2. Nortriptyline 3. Doxepin 4. Imipramine 5. Amitriptyline 6. Trimipramine

Tailing
Eclpse XDB-C8
USP TF (5%) i

	A	B
1.	1.60	1.70
2.	2.00	1.90
3.	1.56	1.56
4.	2.13	1.70
5.	2.15	1.86
6.	1.25	1.25

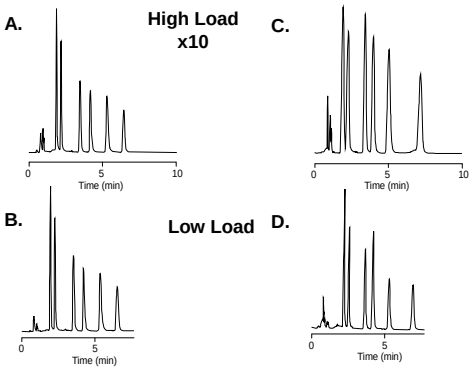

Broadening
Competitive C8
Plates

	C	D
1.	850	5941
2.	815	7842
3.	2776	6231
4.	2539	8359
5.	2735	10022
6.	5189	10725

Tip: Evaluate Both Volume and Mass Loading

Agilent Technologies

Peak Shape: Broad Peaks

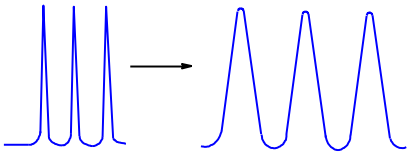

All Peaks Broadened:

- Loss of Column Efficiency.
- Column Void.
- Large Injection Volume.

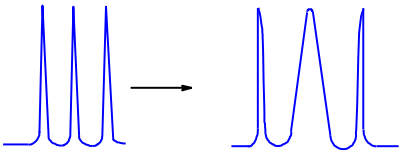

Some Peaks Broadened:

- Late Elution from Previous Sample (Ghost Peak).
  - High Molecular Weight.
  - Sample - Protein or Polymer.

Agilent Technologies

Unknown "Phantom" Peaks

Column: Extend-C18, 4.6 x 150 mm, 5 µm Mobile Phase: 40% 10 mM TEA, pH 11 : 60% MeOH Flow Rate: 1.0 mL/min
Temperature: R.T. Detection: UV 254 Sample: 1. Maleate 2. Pseudoephedrine 3. Chlorpheniramine

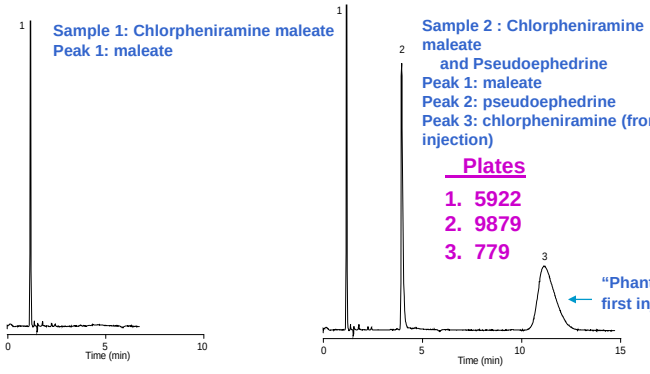

Tip: The extremely low plates for moderately retained peaks are an indication of a very late eluting peak from a preceding run.

Agilent Technologies

Extra-Column Dispersion

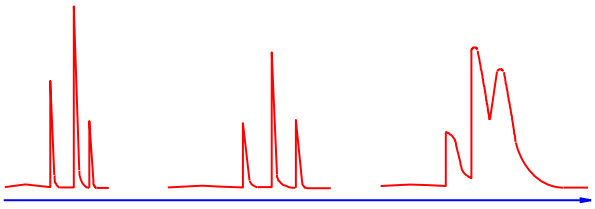

Increasing Extra-Column Volume

- Use short, small internal diameter tubing between the injector and the column and between the column and the detector.
- Make certain all tubing connections are made with matched fittings.
- Use a low-volume detector cell.
- Inject small sample volumes.

Agilent Technologies

Peak Broadening
Extra-Column Volume

Column: StableBond SB-C18, 4.6 x 30 mm, 3.5 µm Mobile Phase: 85% H_2O with 0.1% TFA : 15% ACN Flow Rate: 1.0 mL/min
Temperature: 35°C Sample: 1. Phenylalanine 2. 5-benzyl-3,6-dioxo-2-piperazine acetic acid 3. Asp-phe 4. Aspartame

10 mL extra-column volume

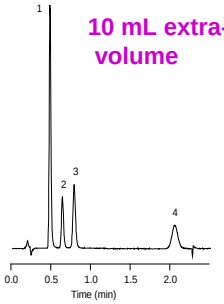

50 mL extra-column volume (tubing)



Agilent Technologies

Tip: Poorly Made HPLC System Connections Can Cause Peak Broadening

The System Has Been Optimized and :

- All Tubing Lengths Are Minimum
- Smallest Diameter Tubing Used
- Proper Flow Cell Volume

Symptom Still Seems to Have Too Much Extra-Column Volume

What Is Wrong?

Have You Made the Connections Properly?

Agilent Technologies

Column Connectors Used in HPLC

Troubleshooting LC Fittings, Part II. J. W. Dolan and P. Upchurch. LC/GC Magazine 6:788 (1988)

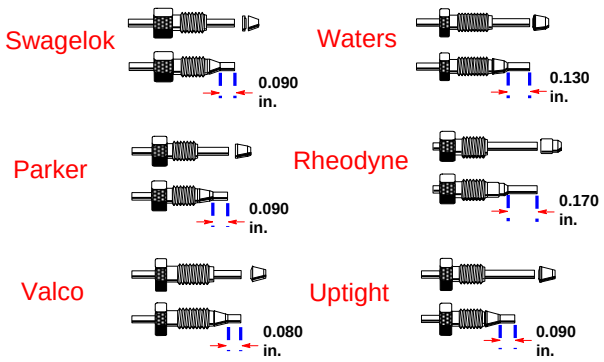

Agilent Technologies

What Happens If the Connections Poorly Made ?

Wrong … too long

Ferrule cannot seat properly

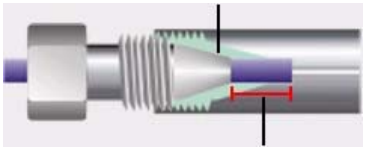

If Dimension X is too long, leaks will occur

Wrong … too short

Mixing Chamber

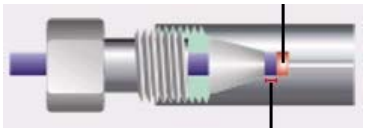

If Dimension X is too short, a dead-volume, or mixing chamber, will occur

Agilent Technologies

Stainless Steel and Polymer Fittings

Which type is used and when?

Stainless Steel (SS) fittings are the best choice for reliable high pressure sealing

- Agilent uses Swagelok type fittings with front and back ferrules – which give best sealing performance – throughout all our LC systems

PEEK (<400b bar System Pressure) fittings are ideal where:

- Connections are changed frequently, i.e. connecting columns
- Pressure is less critical

PolyKetone

- Easy, hand tighten column connection
- **600 bar Pressure Rating** PN: 5042-8957 (10/pk)
- Fits to SS Tubing

Agilent Technologies

Changes in Retention Can Be Chemical or Physical

May be caused by:

- Column aging
- Column contamination
- Insufficient equilibration
- Poor column/mobile phase combination
- Change in mobile phase
- Change in flow rate
- Different Gradient Delay Volumes

Agilent Technologies

Column Aging/Equilibration Causes Retention/Selectivity Changes

Column 1 - Initial



Column 1 - Next Day



Column 1 - After Cleaning with 1% H_3PO_4 /Equilibration



- The primary analyte was sensitive to mobile phase aging/ conditioning of the column
- The peak shape was a secondary issue (metal chelating compound) resolved by “de-activating” the active metal contamination

Agilent Technologies

Metal Sensitive Compounds Can Chelate

Hint: Look for Lone Pair of Electrons on :O: or N Which Can Form 5 or 6 Membered Ring with Metal



Salicylaldehyde **6-membered ring complex**

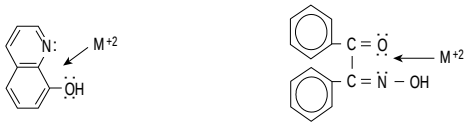

8-hydroxyquinoline
5-membered ring complex

a-benzoinoxomine
5-membered ring complex

Agilent Technologies

Acid Wash Can Improve Peak Shape

Before Acid Wash



After Acid Wash
50 – 100 mLs 1% H_3PO_4





Tf: 3.7

Columns: ZORBAX SB-Phenyl 4.6 x 150 mm
Mobile Phase: 75% 25 mM ammonium phosphate buffer
25% ACN
Flow Rate: 1.0 mL/min.
Temperature: RT
Sample Size: 5 mL



Tf: 1.2

• A 1% H_3PO_4 solution is used on SB columns, 0.5 % can be used on endcapped columns.

Agilent Technologies

Example: Change in Retention/Selectivity

Unintended Mobile Phase Variation

Tip: The Source of the Problem is Often Not the Obvious Change

Column 1



Column 2



Column 2 - Fresh mobile phase



"I have experimented with our mobile phase, opening new bottles of all mobile phase components. When I use all fresh ingredients, the problem ceases to exist, and I have narrowed the problem to either a bad bottle of TEA or phosphoric acid. Our problem has been solved."

Tip: Dwell Volume Differences Between Instruments Can Cause Changes in Retention and Resolution

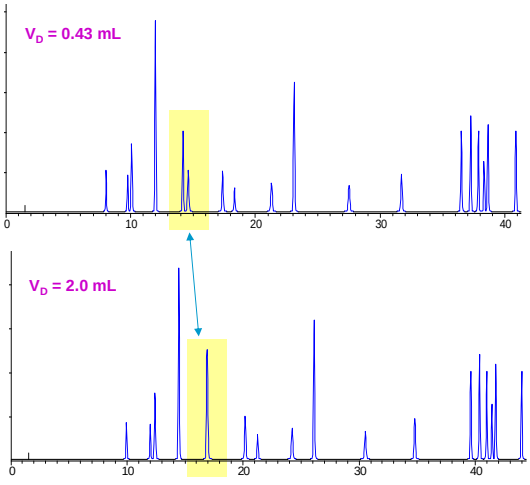

Column: **ZORBAX Rapid Resolution Eclipse XDB-C8 4.6 x 75 mm, 3.5 µm**

Mobile Phase: Gradient, 0 - 100 %B in 52.5 min.
A: 5/95 methanol/ 25 mM phosphate pH 2.50
B: 80/20 methanol/25 mM phosphate pH 2.50

Flow Rate: 0.5 mL/min

Temperature: 25°C

Injection: 5 µL

Detection: 250 nm

Sample: Mixture of antibiotics and antidepressants

Upper trace simulates actual run data entered into DryLab® 3.0 software

Lower trace is simulated chromatogram for larger V_D

Trick: Measure and Correct for Dwell Volume (V_D)

If $V_{D1} > V_{D2}$

Compensate for longer V_{D1} by adding an isocratic hold to V_{D2}, such that Hold + V_{D2} = V_{D1}

If $V_{D1} < V_{D2}$

Delay injection, such that V_{D2} - delay = V_{D1}

Mobile Phase pH and pH Buffers
Why Are These So Important in HPLC?

- pH Effects Ionization
  - Silica Surface of Column
  - Sample Components of Interest
- Buffers
  - Resist Changes in pH and Maintain Retention
  - Improve Peak Shape for Ionizable Compounds
- Effects Column Life
  - Low pH strips Bonded Phase
  - High pH Dissolves Silica

Minimize Change in Retention/Selectivity
Lot-to-Lot

Evaluate:

- All causes of column-to-column change*
- Method ruggedness (buffers/ionic strength)
- pH sensitivity (sample/column interactions)

*All causes of column-to-column change should be considered first, especially when only one column from a lot has been tested.

Agilent Technologies

Lot-to-Lot Selectivity Change Related to pH Choice

pH 4.5 - Lot 1



pH 3.0 - Lot 1



pH 4.5 - Lot 2



pH 3.0 - Lot 2



- pH 4.5 shows selectivity change from lot-to-lot for basic compounds
- pH 3.0 shows no selectivity change from lot-to-lot
- Indication of poorly controlled ionization

Agilent Technologies

Why Worry About pH?
pH, pKa and Weak Acids

$$RCOOH \rightleftharpoons RCOO^- + H^+ \qquad K_a = \frac{[RCOO^-][H^+]}{[RCOOH]}$$



$K_a = 6.4 \times 10^{-5}$
$pK_a = 4.2$

At pH 4.2 – the sample exists as benzoic acid and the benzoate ion in a ratio of 1:1. Peak shape can be poor
At pH 5.2 – 91% of the sample exists as the benzoate ion. RP retention decreases.
At pH 3.2 – 91% of the sample exists as benzoic acid. RP retention increases.

Agilent Technologies

Effect of pH on Peak Shape at or Near the Sample pK_a

Column: ZORBAX SB-C8 4.6 x 150 mm, 5 mm Mobile Phase: 40% 5 mM KH_2PO_4: 60% ACN
Flow Rate: 1.0 mL/min. Temperature: RT

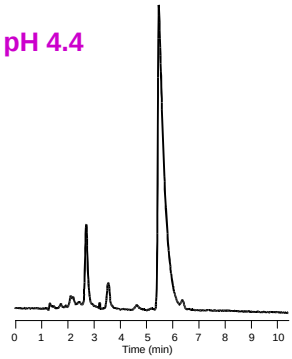

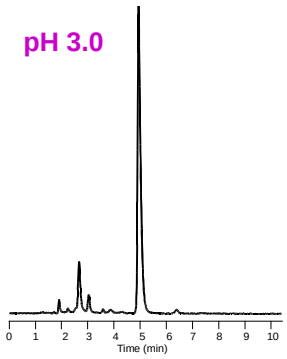



Ibuprofen
$pK_a = 4.4$

- Inconsistent and tailing peaks may occur when operating close to an analyte pKa and should be avoided.

Agilent Technologies

Why Worry About pH?
pH, pKa and Weak Bases

$$R_3NH^+ \rightleftharpoons R_3N + H^+$$

$$K_a = \frac{[R_3N][H^+]}{[R_3NH^+]}$$

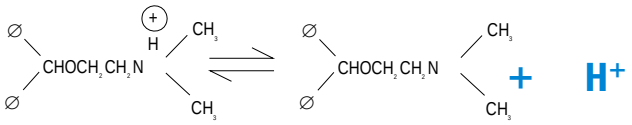

$K_a = 1 \times 10^{-9}$
$pK_a = 9$

At pH 9 – the sample exists as protonated and unprotonated diphenhydramine in a ratio of 1:1. Peak shape can be poor.
At pH 10 – 91% of the sample exists as unprotonated diphenhydramine.
At pH 8 – 91% of the sample exists as protonated diphenhydramine.

Agilent Technologies

pH vs. Selectivity for Acids and Bases

Column: Nucleosil-C18
Mobile Phase: 45% ACN/55% phosphate buffer
Sample: Bile Acids

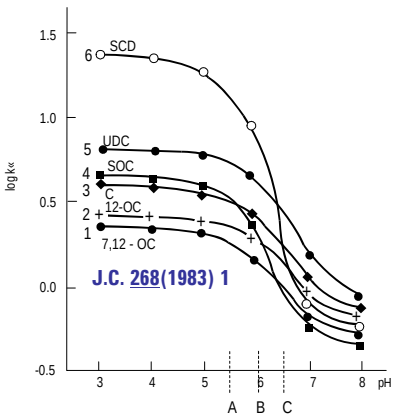

Column: mBondapak-C18
Mobile Phase: 60% 25 mM phosphate buffer
40% Methanol

1. Salicylic acid
2. Phenobarbital
3. Phenacetin
4. Nicotine
5. Methamphetamine

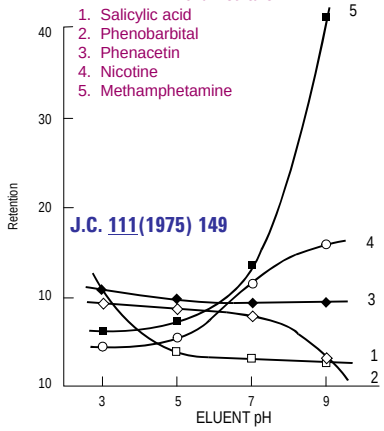

• **Retention and selectivity can change dramatically when pH is changed.**

Agilent Technologies

Importance of pH and Buffers
A Practical Example

- Why the Sample Dictates Use
- What Happens When Buffer Used Effectively
- What Happens When Buffer Ignored or Used Improperly

Agilent Technologies

Importance of pH and Buffers - A Practical Example
Optimized Isocratic Conditions for Cardiac Drugs

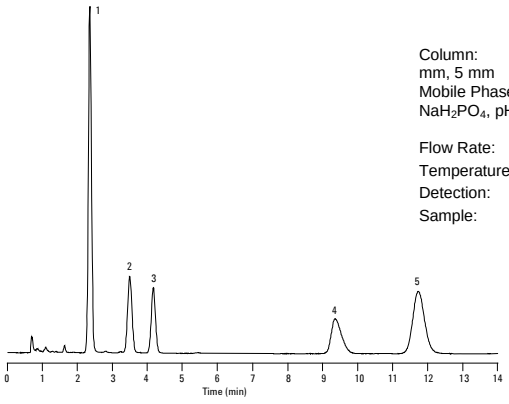

Column: StableBond SB-C18, 4.6 x 150 mm, 5 mm
Mobile Phase: 45% 25 mM NaH_2PO_4, pH 3.0
55% MeOH
Flow Rate: 2.0 mL/min.
Temperature: 35°C
Detection: UV 254 nm
Sample: Cardiac Drugs
1. Diltiazem
2. Dipyridamole
3. Nifedipine
4. Lidoflazine
5. Flunarizine

Agilent Technologies

I Don’t Have Time to Make Buffers or Adjust pH …

Column: **StableBond SB-C18**
4.6 x 150 mm, 5 mm
Mobile Phase: A: 20% H_2O
B: 80% MeOH
Flow Rate: 1.0 mL/min.
Temperature: 35°C
UV Detection: 254 nm
Sample: Cardiac Drugs

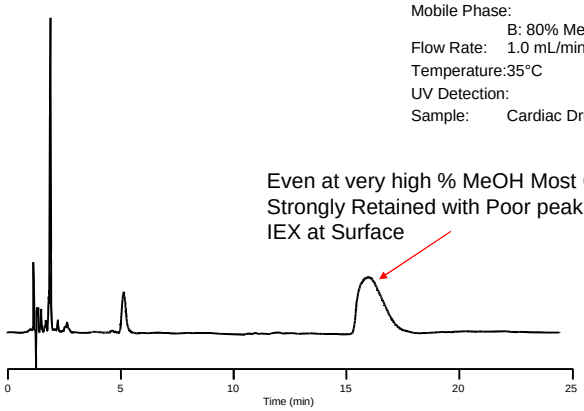

- **Buffers are critical to good retention and peak shape in many separations.**

Agilent Technologies

What If You Work Outside the Buffer Range?

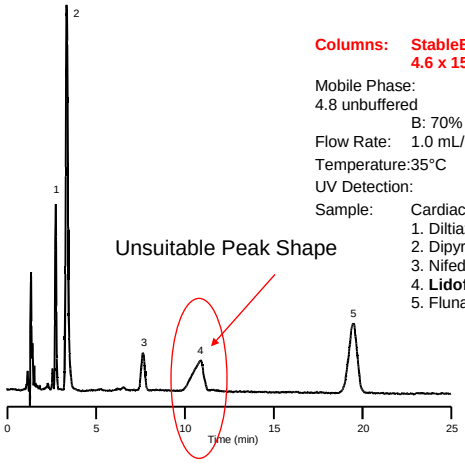

Columns: **StableBond SB-C18**
4.6 x 150 mm, 5 mm
Mobile Phase: A: 30% 25 mM NaH_2PO_4, pH 4.8 unbuffered
B: 70% MeOH
Flow Rate: 1.0 mL/min.
Temperature: 35°C
UV Detection: 254 nm
Sample: Cardiac Drugs
1. Diltiazem
2. Dipyridamole
3. Nifedipine
4. **Lidoflazine**
5. Flunarizine

Agilent Technologies

Don’t Forget - Match Column to pH of Mobile Phase for Maximum Column Lifetime

low pH and high temperature (pH 0.8, 90°C)

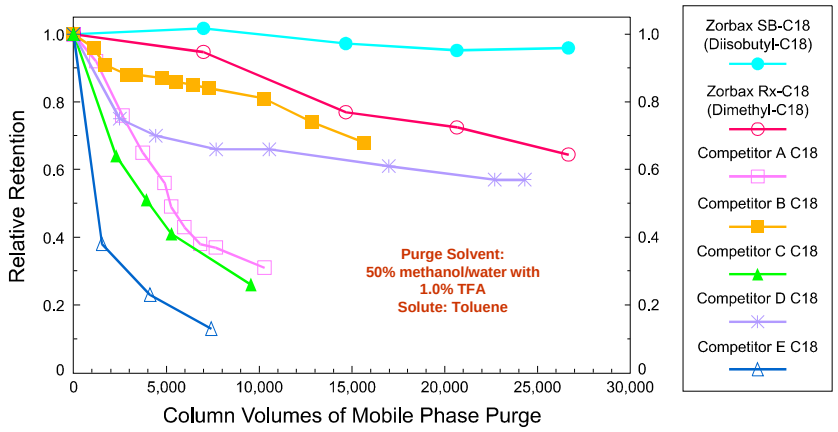

Kirkland, J.J. and J.W. Henderson, Journal of Chromatographic Science, 32 (1994) 473-480.

Don’t Forget - Match Column to pH of Mobile Phase for Maximum Column Lifetime

High pH and Room Temperature (pH 11 RT)

Mobile Phase: 50%ACN: 50% Water : 0.2% TEA (~ pH 11)

Initial

After 30 injections

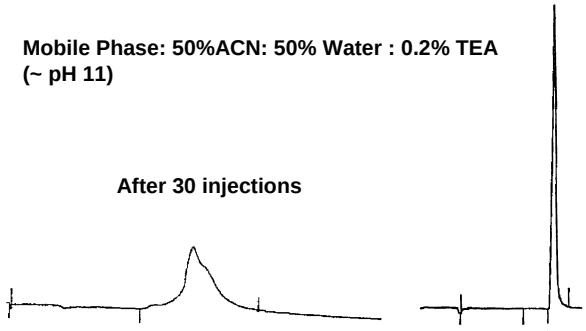

Tip: Use Columns Designed for chosen pH

Detection Issues

Recognize Where the Problem Originates

- Is it a consequence of technique?
- Is It expected due to use of certain mobile phase components?
- Can it be corrected by adjusting detector parameters?
- Answers Will Help Find a Solution!

Let's Explore Some Problems and Solutions

Agilent Technologies

Peak Shape: Negative Peaks

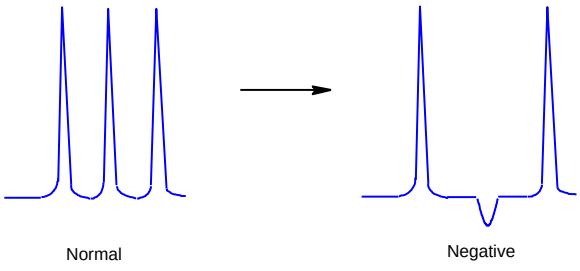

Causes:

- Absorbance of sample is less than the mobile phase.
- Equilibrium disturbance when sample solvent passes through the column.
- Normal with Refractive Index Detectors.

Agilent Technologies

Ghost Peaks

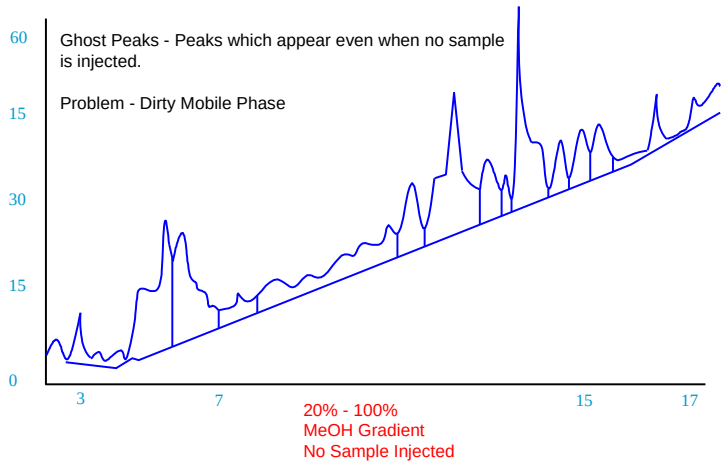

Agilent Technologies

Noisy Baselines

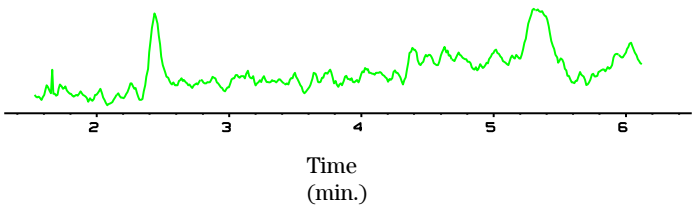

Possible Causes:

- Dirty Flow Cell
- Detector Lamp Failing
- Pulses from Pump if Periodic
- Temperature Effects on Detector
- Air Bubbles passing through Detector

Agilent Technologies

Drifting Baselines

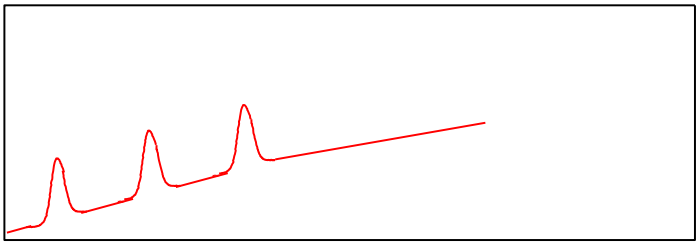

- Gradient Elution
- Temperature Unstable (Refractive Index Detector)
- Contamination in Mobile Phase
- Mobile Phase Not in Equilibrium with Column
- Contamination Bleed in System

Agilent Technologies

Chromatographic Results with "Wrong" Lamp at 214 nm Wavelength

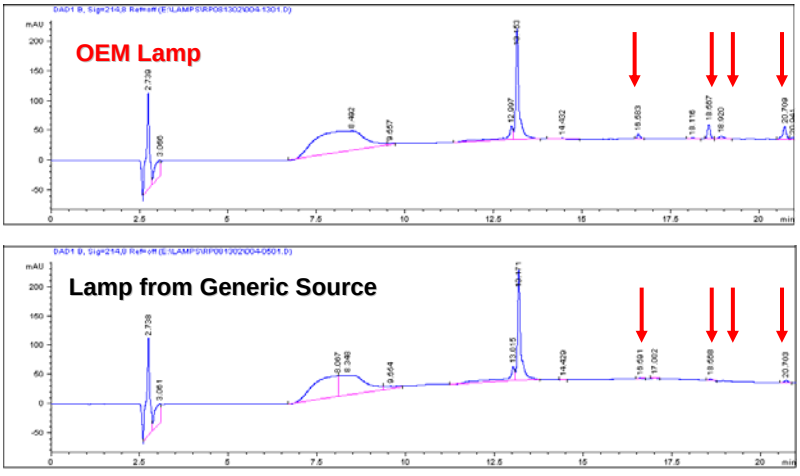

Tip: Could also be a symptom of aging lamp

Agilent Technologies

Expanded View of Chromatographic Results
Generic Source Lamp at 214 nm Wavelength

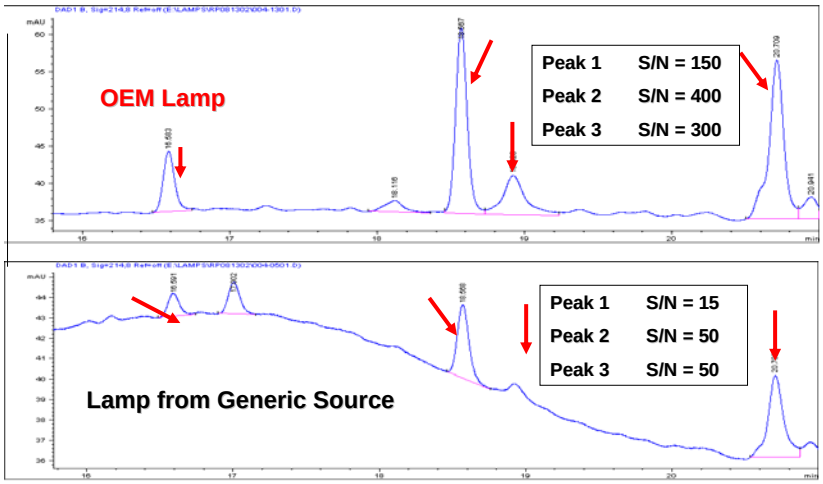

Tip: Poor S/N makes it difficult to detect low level impurities

Agilent Technologies

Effect of Detector Response Time

The System is operating well-the settings were poorly made!

Slow Data Rates Can Hinder Impurity Detection and Reduce Sensitivity

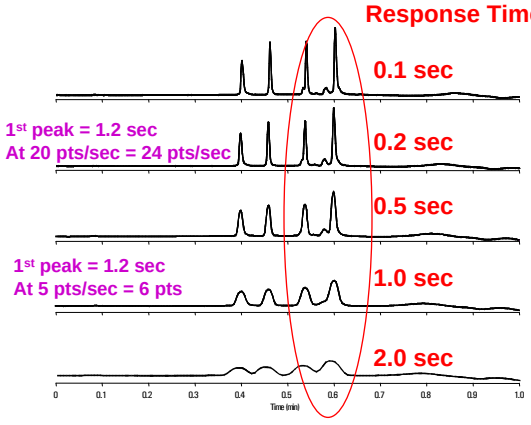

Agilent 1100 DAD
Agilent 1100 WPS with ADVR

Column: **Poroshell 300SB-C18**
2.1 x 75 mm, 5 mm

Mobile Phase:
A: 95% H_2O, 5% ACN with 0.1% TFA
B: 5% H_2O, 5% ACN with 0.1% TFA

Flow Rate: 2 mL/min

Temperature: 70°C

Detector: UV 215 nm

Piston stroke: 20

Sample:
1. Neurotensin 3. Lysozyme
2. RNaseA 4. Myoglobin

- Tip: Adjust the response rate of your detector for best peak detection.

Agilent Technologies

Conclusions

HPLC column problems are evident as

- High pressure (prevention better than the cure)
- Undesirable peak shape
- Changes in retention/selectivity

Often these problems are not associated with the column and may be caused by instrument and chemistry issues.

- pH of mobile Phase
- Instrument Connections
- Detector Settings
- Metal Contamination

Start With the Correct Questions

- Find the Answers
- The Answers will Lead to Solutions